Replacement Sheet

Fig.1




Fig.2 (Prior Art)


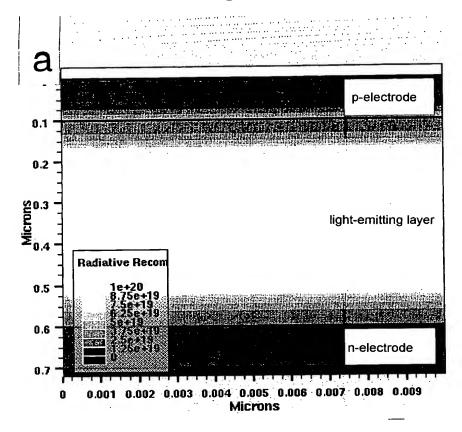


Fig.3



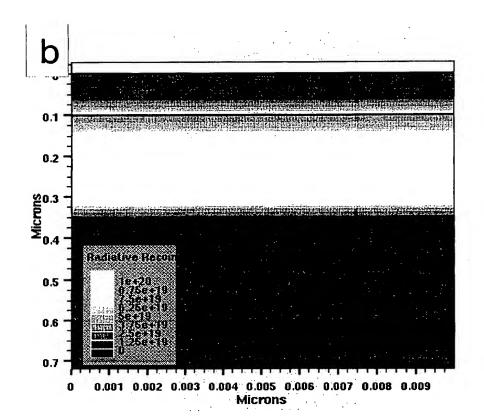
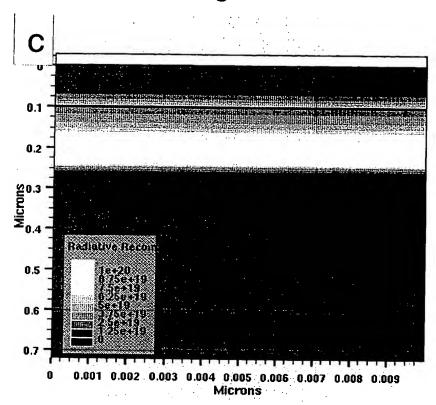
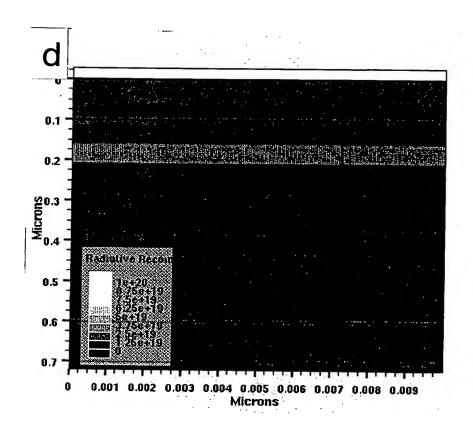


Fig.4







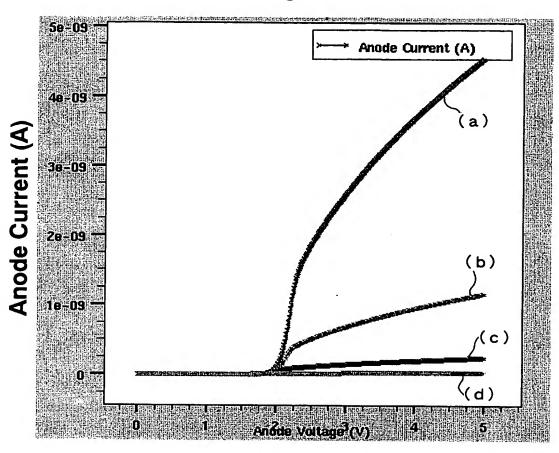
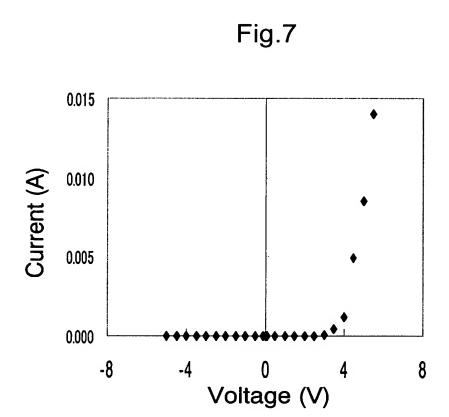


Fig.6 5 1 5 2 5 7 QUADPLEX HARMONICS OSCILLATOR YAG LASER BANDPASS FILTER (265nm) IRIS OSCILLATOR TRIGGER SYNO. OUTPUT R=500Ω XYZ 8 -STAGE 5 4 TRIG. POMER MPLIFIER 5 3 EVENT OSCILLO SCOPE PERSONAL COMPUTER PROBE BIAS

-5 5



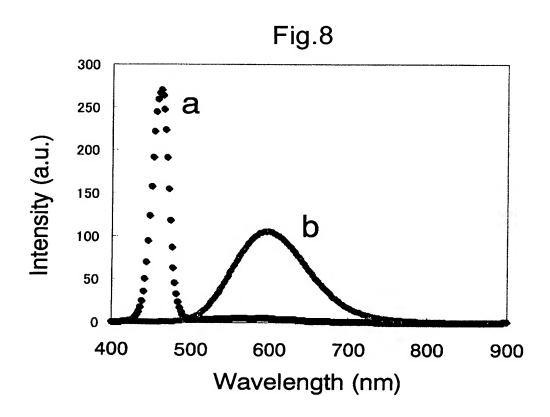


Fig.9

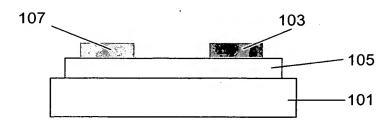


Fig.10

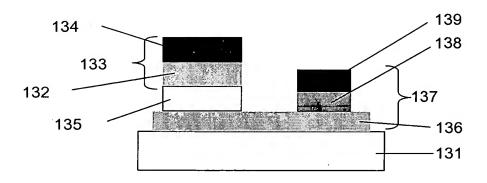


Fig.11

